


# First wearable device can monitor jaundice-causing bilirubin and vitals in newborns

4 March 2021

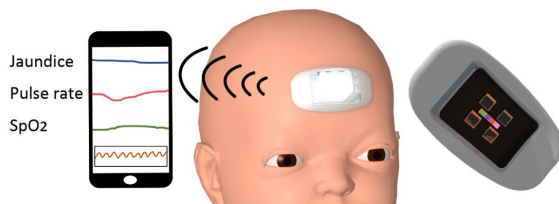

Schematic of neonatal wearable device for detecting jaundice and vitals. Credit: Yokohama National University

Researchers in Japan have developed the first wearable devices to precisely monitor jaundice, a yellowing of the skin caused by elevated bilirubin levels in the blood that can cause severe medical conditions in newborns. Jaundice can be treated easily by irradiating the infant with blue light that breaks bilirubin down to be excreted through urine. The treatment itself, however, can disrupt bonding time, cause dehydration and increase the risks of allergic diseases. Neonatal jaundice is one of the leading causes of death and brain damage in infants in low- and middle-income countries.

To address the tricky balance of administering the precise amount of [blue light](#) needed to counteract the exact levels of [bilirubin](#), researchers have developed the first wearable sensor for newborns that is capable of continuously measuring bilirubin. In addition to bilirubin detection, the device can simultaneously detect pulse rate and blood oxygen saturation in real time.

Led by Hiroki Ota, associate professor of mechanical engineering in Yokohama National University's Graduate School of System

Integration, and Shuichi Ito, professor of department of Pediatrics in Yokohama City University's Graduate School of Medicine, the team published their results on March 3 in *Science Advances*.

"We have developed the world's first wearable multi-vital device for newborns that can simultaneously measure neonatal [jaundice](#), blood oxygen saturation and pulse rate," Ota said, noting that jaundice occurs in 60 to 80% of all newborns. "The real-time monitoring of jaundice is critical for neonatal care. Continuous measurements of [bilirubin levels](#) may contribute to the improvement of quality of phototherapy and patient outcome."

Currently, [medical professionals](#) use handheld bilirubinometers to measure bilirubin levels, but there is not a device that can simultaneously measure jaundice and vitals in real time.



Actual wearable device. Credit: Yokohama National University

"In this study, we succeeded in miniaturizing the device to a size that can be worn on the forehead

of a newborn baby," Ota said. "By adding the function of a pulse oximeter to the device, multiple vitals can easily be detected."

Held to the baby's forehead by a silicone interface, the device has a lens capable of efficiently transmitting lights to neonatal skin via battery-powered light-emitting diodes, commonly known as LEDs.

"At the present stage, coin cell batteries are used, and the overall shape is very thick," Ota said. "In the future, it will be necessary to further reduce the thickness and weight by using thin-film batteries and organic materials."

The researchers tested the device on 50 babies, and they found that the device is not currently accurate enough to suffice for clinical decision-making. According to Ota, they will reduce the thickness and increase the flexibility of the device, as well as improve the silicone interface to facilitate better skin contact.

In the future, the researchers plan to develop a combined treatment approach that pairs a wearable bilirubinometer with a phototherapy [device](#) to optimize the amount and duration of light therapy based on continuous measurements of bilirubin levels.

**More information:** Go Inamori et al, Neonatal wearable device for colorimetry-based real-time detection of jaundice with simultaneous sensing of vitals, *Science Advances* (2021). [DOI: 10.1126/sciadv.abe3793](#)

Provided by Yokohama National University

APA citation: First wearable device can monitor jaundice-causing bilirubin and vitals in newborns (2021, March 4) retrieved 26 August 2022 from <https://medicalxpress.com/news/2021-03-wearable-device-jaundice-causing-bilirubin-vitals.html>

*This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.*